


# SwiftMR™

AI-Powered MRI Enhancement Solution  
Faster Imaging, Exceptional Quality

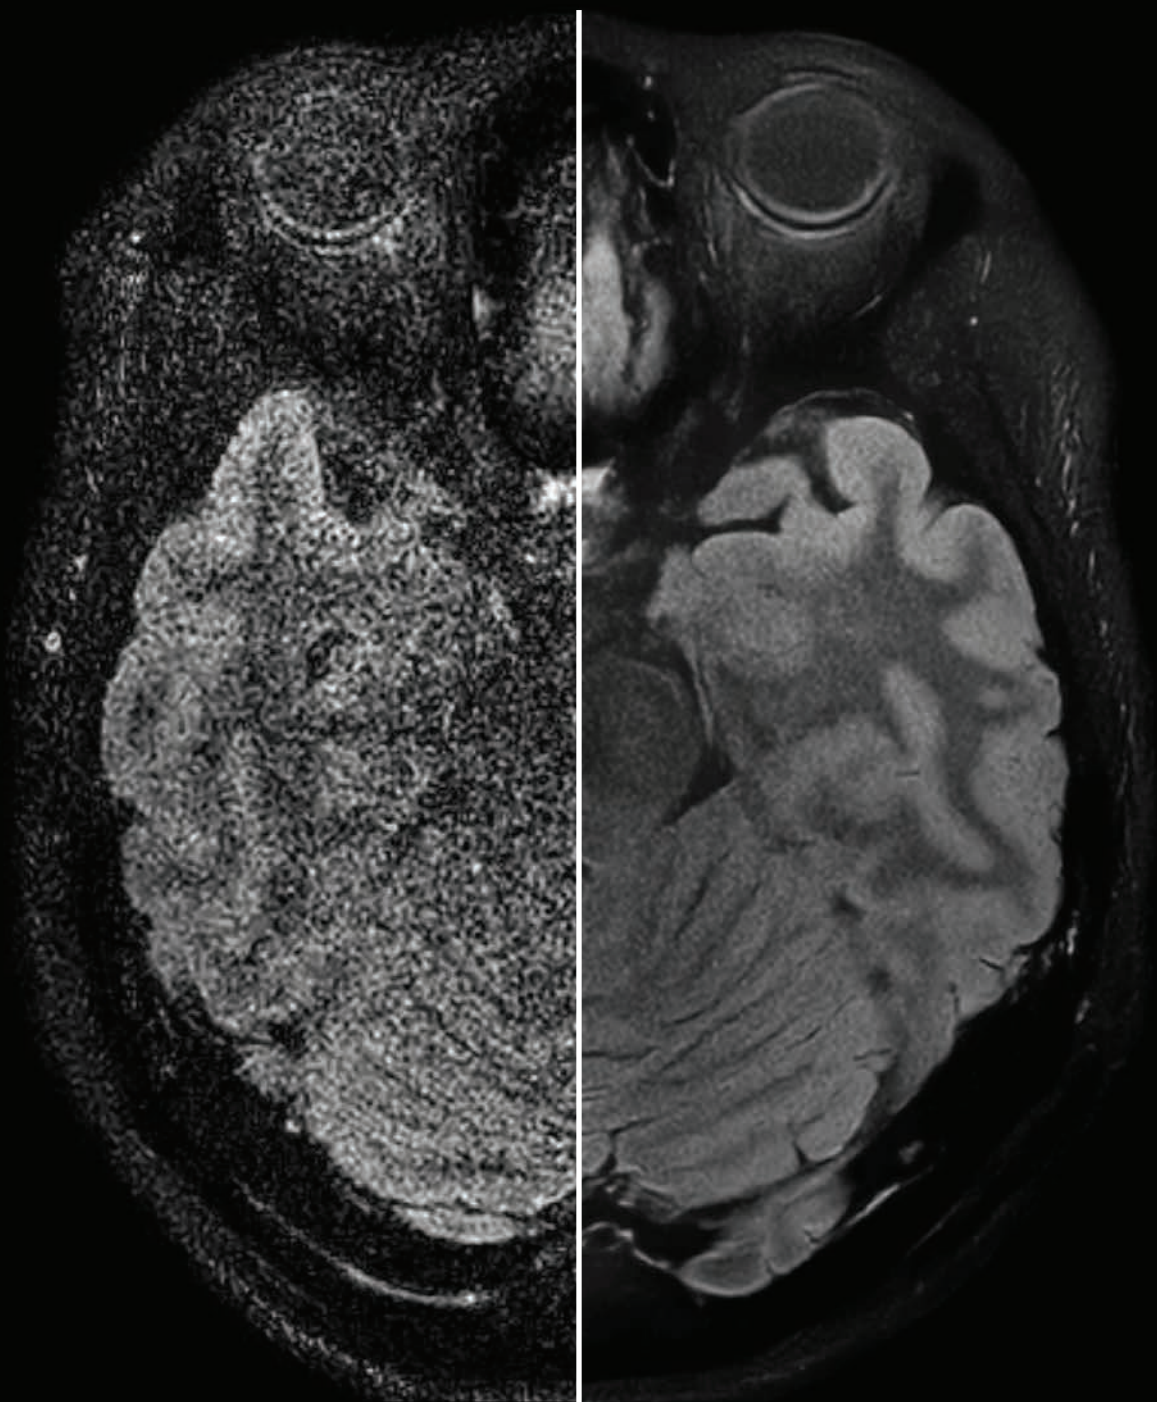

## Introducing SwiftMR™

# The Next Generation MRI Enhancement Software

SwiftMR™ is a transformative solution that enables MRI scan time reduction, enhancing patient comfort without sacrificing image quality. Developed with a cutting-edge deep learning model, SwiftMR™ is designed to integrate seamlessly with existing MRI systems.

### Enhanced Efficiency

Proven to enable scan time reduction by up to 50%\*, significantly boosting patient throughput.



### Exceptional Image Quality

Enhances image quality, making scans from even legacy systems clearer and more detailed.




### Comprehensive Coverage

FDA-510(K) clearance ensures compatibility with all body parts, sequences and manufacturers.



## How SwiftMR™ works

Our team will optimize MRI protocols to accelerate scans, initially producing faster yet noisy and blurry images. SwiftMR™'s deep learning model is then employed to enhance the accelerated scans, effectively transforming them into high-quality images.

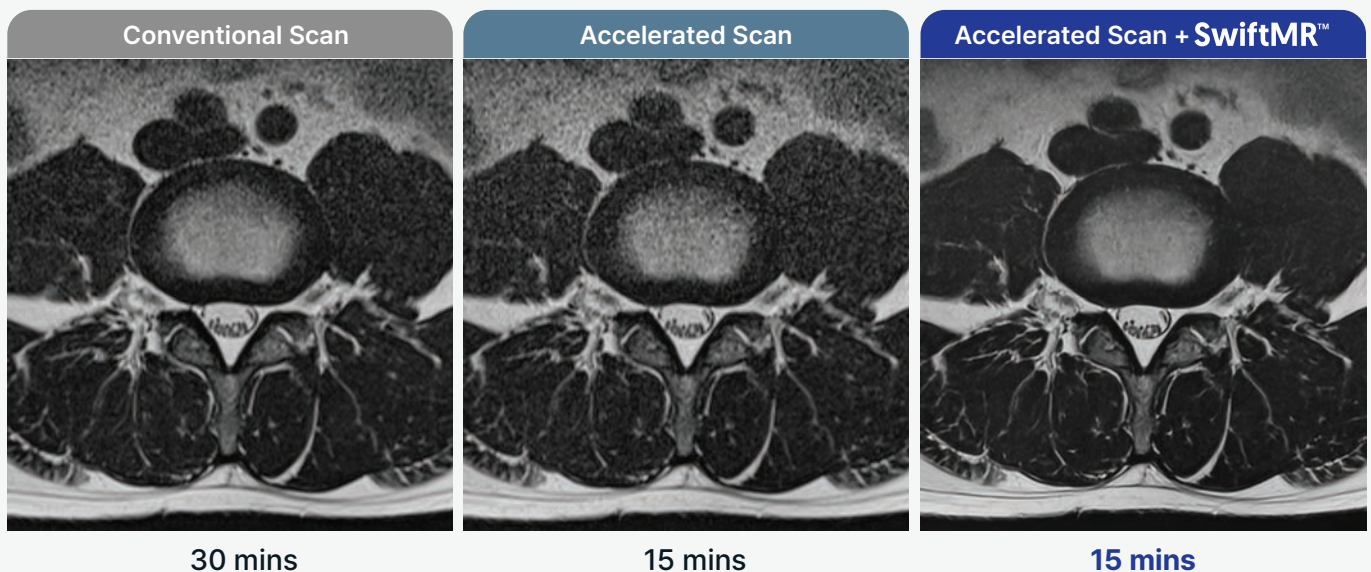

USA	Europe	KOREA
<b>FDA 510(k)-cleared</b> Class II	<b>CE</b> <sub>2460</sub> Class IIa, MDR	<b>KOREA MFDS approved</b> Class 1
Quality Management System		Information Security
ISO 13485:2016 / EN ISO 13485:2016 certified GMP, MDSAP certified		HIPAA-compliant, GDPR-compliant ISO 27001, 27017, 27018 certified

\* For investigational purposes in countries outside of the United States, South Korea, Canada, Brazil, Japan, Taiwan, Malaysia, Saudi Arabia, UAE, Thailand, Vietnam, and Indonesia. FDA 510(k)-cleared to support images with scan time reduction by up to 50% in the United States.

SwiftMR™ Delivers Real Results:

# Boost your Productivity and Efficiency

SwiftMR™ enables radiology practices to achieve a new level of productivity and efficiency with MRI scans. Reducing MRI scan time increases patient throughput, unlocking opportunities for revenue growth through increased MRI utilization.

With SwiftMR™, GK Medical in Illinois achieved **37% more scans with 40% shorter scan time\***

## Scan time changes


Avg. **40%** scan time reduction

Body part	Scan time (Before)	Scan time (After)	Reduction
Prostate	39:17	21:17	<b>49%</b>
C-spine	23:13	13:41	<b>41%</b>
L-spine	18:47	12:03	<b>36%</b>
Brain	37:04	25:01	<b>33%</b>

\*Results on Siemens Trio 3T

## MRI scan volume

**37%** scan volume increase

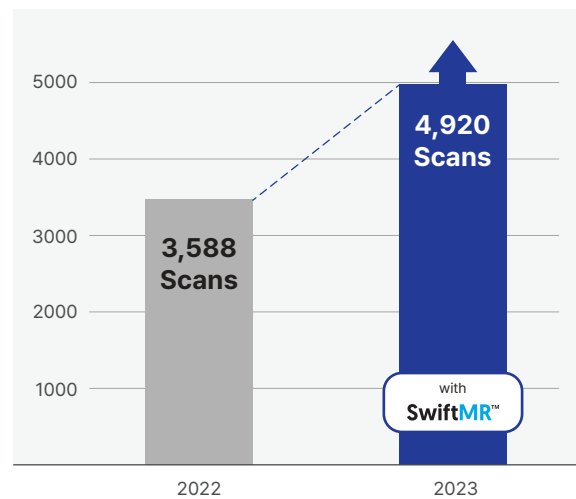

## SwiftMR™ 's Comprehensive Coverage\*\*

What sets us apart is our thoughtful approach to designing products for radiology practices. Our products cater to a diverse range of needs, providing comprehensive coverage.



Ages  
**All ages**



Body parts  
**All body parts**



Field strength  
**3.0T or lower**



Pulse sequence  
**All pulse sequences**



Manufacturers  
**All MRI manufacturers**

\* Numbers based on data from a single location and individual results may vary

\*\* Supported body parts, pulse sequence, field strength, patient population and MRI manufacturers may vary by country



# SwiftMR™ Enables Faster Scans


SwiftMR™ enables scan time reduction by up to 50%\*, while preserving image quality.

---


## Brain MRA

1.5T  
Philips  
Ingenia

3D TOF  
Ⓐ 0.6×0.8×1.2 mm  
Ⓑ 0.6×0.8×1.2 mm  
MIP

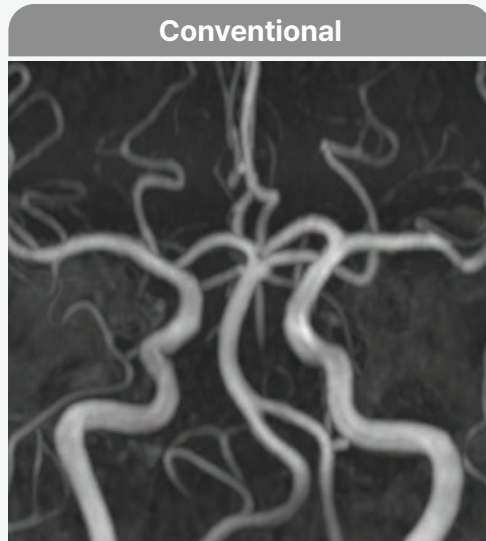

Scan time 04:42

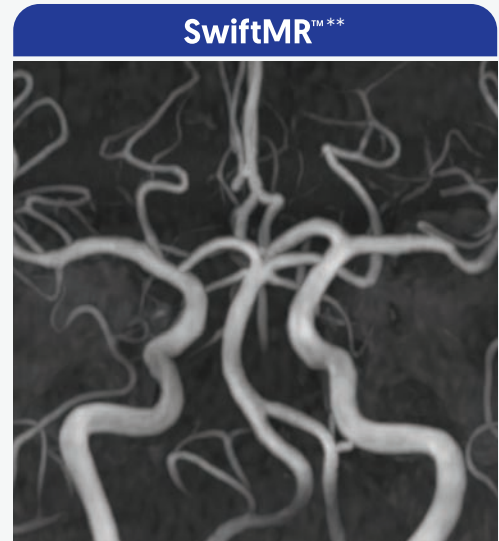


Scan time 02:28

---


## Brain T1WI

3.0T  
GE  
Discovery MR750w

3D BRAVO  
Ⓐ 1.0×1.0×1.0 mm  
Ⓑ 1.0×1.0×1.0 mm

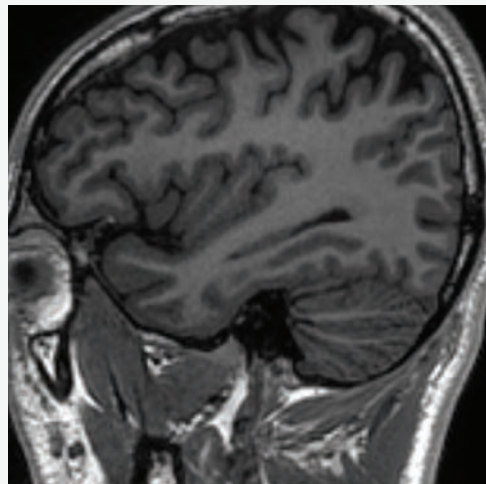

Scan time 04:11

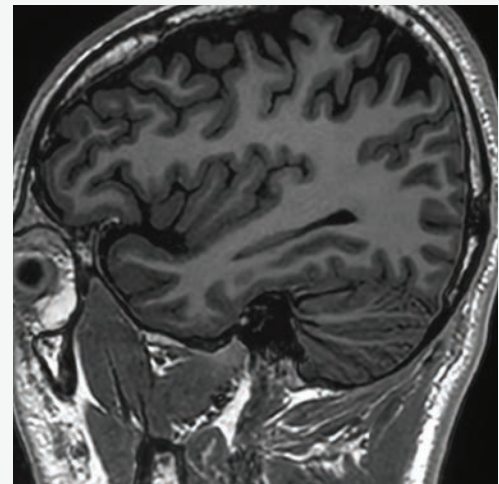


Scan time 01:55

---


## Brain T2WI

3.0T  
Siemens  
MAGNETOM Skyra

2D TSE  
Ⓐ 0.4×0.4×5.0 mm  
Ⓑ 0.4×0.4×5.0 mm

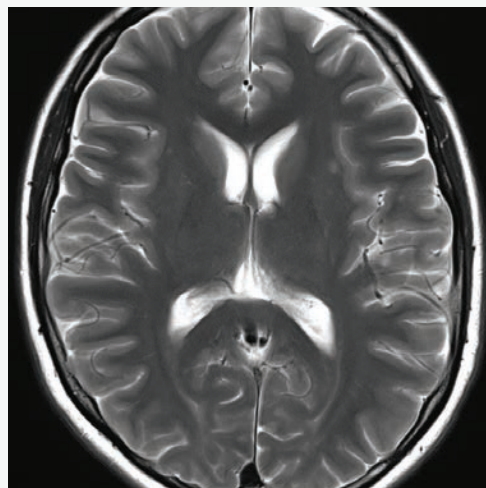

Scan time 02:22

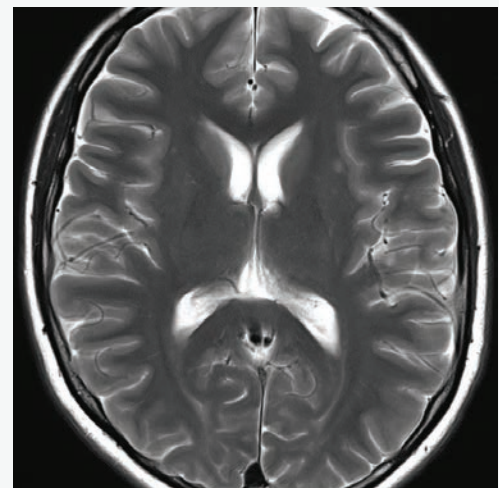

Scan time 01:09

---


\* FDA 510(k)-cleared for Standard of Care(SOC) and reduced scan time MR images for all body parts.

\*\* For investigational purposes in countries outside of the United States, South Korea, Canada, Brazil, Japan, Taiwan, Malaysia, Saudi Arabia, UAE, Thailand, Vietnam, and Indonesia. FDA 510(k)-cleared to support images with scan time reduction by up to 50% in the United States.

See more images




### Conventional

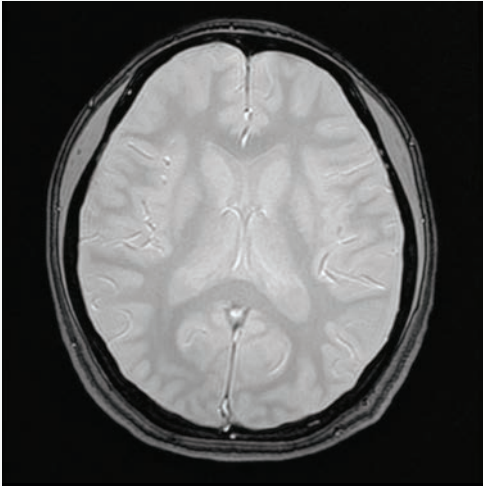

Scan time 03:17

### SwiftMR™\*

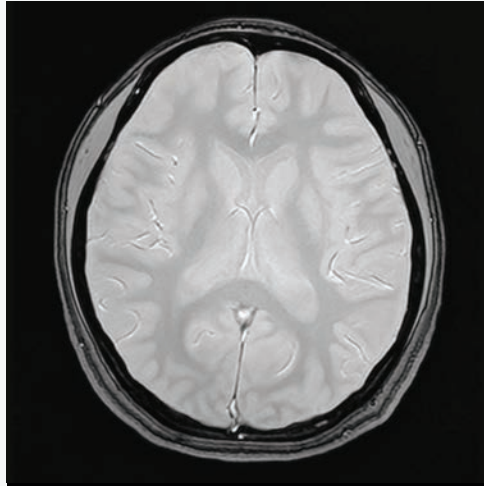

Scan time 01:40


### Brain T2\*WI

1.5T  
GE  
Signa HDxt

2D GRE  
Ⓐ 0.9×1.1×5.0 mm  
Ⓑ 0.9×1.1×5.0 mm



Scan time 03:10

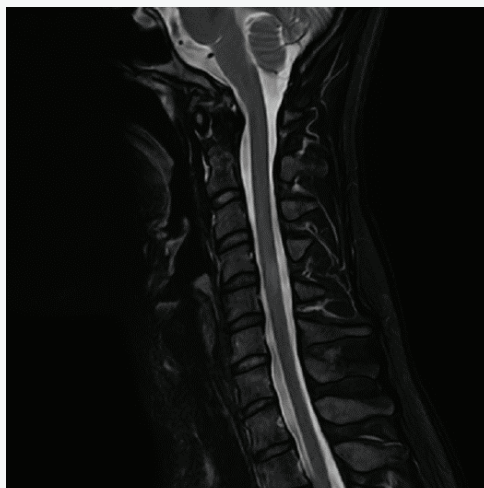


Scan time 01:41

### C-Spine Sagittal T2WI

3.0T  
GE  
Discovery MR750

2D FSE  
Ⓐ 0.4×0.4×3.0 mm  
Ⓑ 0.4×0.4×3.0 mm

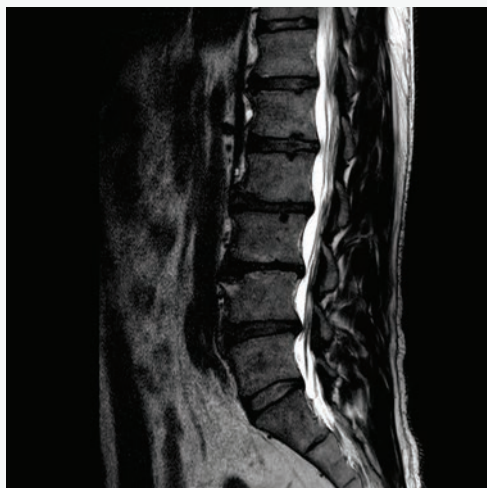

Scan time 06:08



Scan time 00:44

### L-Spine T2WI

3.0T  
Philips  
Ingenia CX

2D TSE  
Ⓐ 0.4×0.9×3.0 mm  
Ⓑ 0.6×1.1×3.0 mm




---


## L-Spine T2WI

1.5T  
Siemens  
MAGNETOM Essenza

2D TSE  
Ⓐ 0.6×0.8×4.0 mm  
Ⓑ 0.6×0.8×4.0 mm

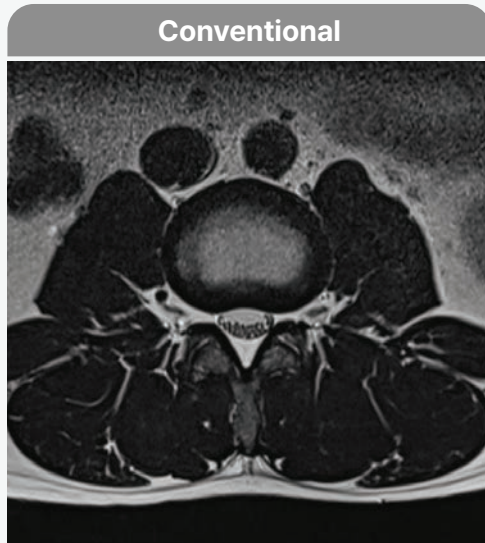

Scan time 03:00

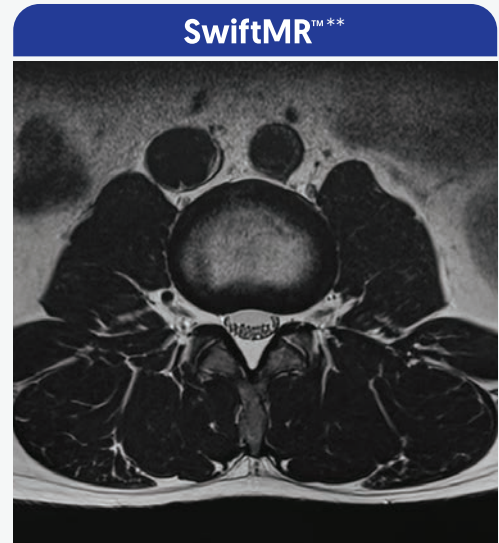


Scan time 01:28

---


## Shoulder PDWI FS

1.5T  
Siemens  
MAGNETOM Essenza

2D TSE  
Ⓐ 0.6×0.8×3.0 mm  
Ⓑ 0.6×0.8×3.0 mm

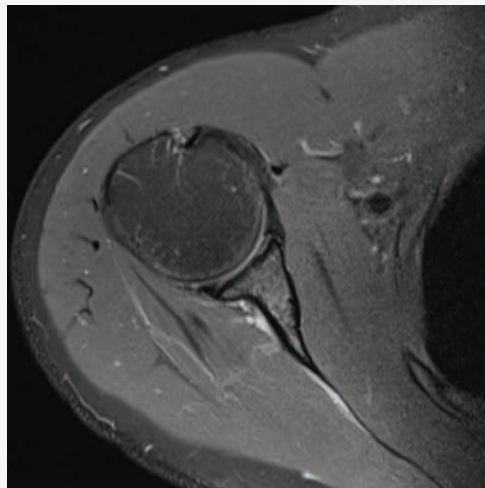

Scan time 02:51

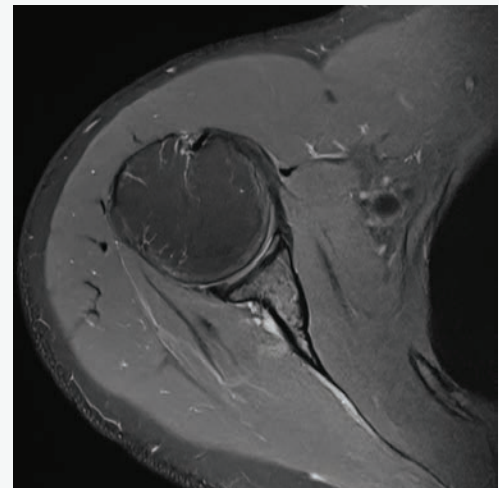

Scan time 01:27

---

## Wrist T2WI FS

3.0T  
GE  
SIGNA Premier

2D FSE  
Ⓐ 0.3×0.4×2.0 mm  
Ⓑ 0.3×0.4×2.0 mm



Scan time 03:19



Scan time 01:49

---


\* FDA 510(k)-cleared for Standard of Care(SOC) and reduced scan time MR images for all body parts.

\*\* For investigational purposes in countries outside of the United States, South Korea, Canada, Brazil, Japan, Taiwan, Malaysia, Saudi Arabia, UAE, Thailand, Vietnam, and Indonesia. FDA 510(k)-cleared to support images with scan time reduction by up to 50% in the United States.

See more images




### Conventional

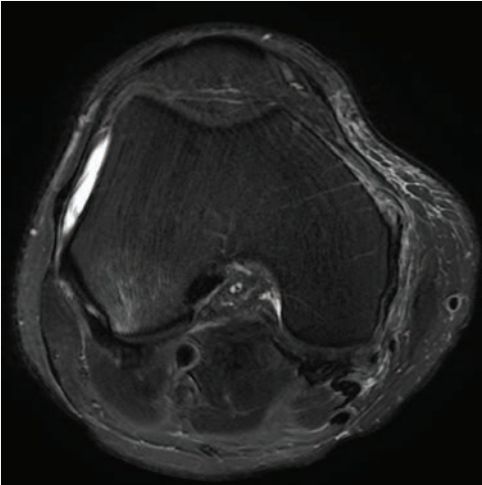

Scan time 03:19

### SwiftMR™\*

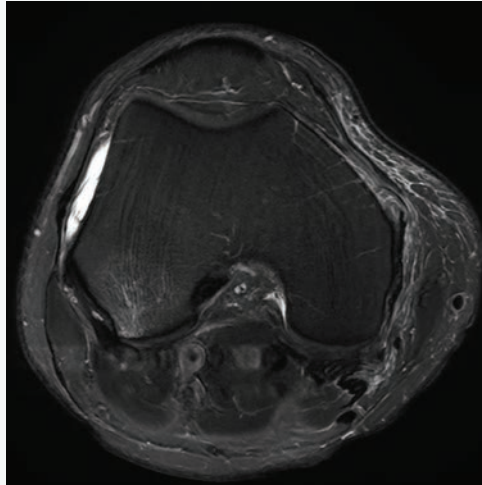


Scan time 01:49

### Knee T2WI FS

3.0T  
GE  
Discovery MR750

2D FSE  
Ⓐ 0.4×0.4×3.0 mm  
Ⓑ 0.4×0.4×3.0 mm

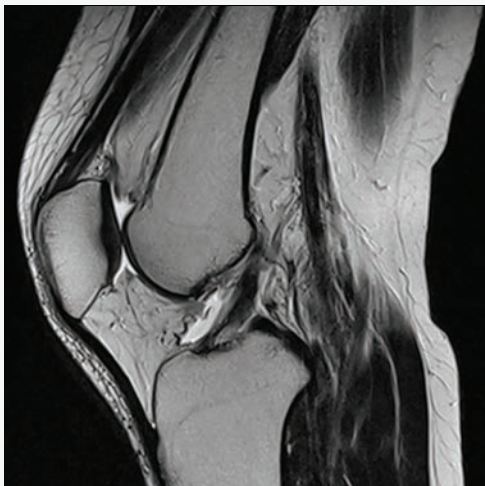

Scan time 03:15



Scan time 01:47


### Knee T2WI

1.5T  
Siemens  
MAGNETOM Essenza

2D TSE  
Ⓐ 0.5×0.6×3.0 mm  
Ⓑ 0.5×0.6×3.0 mm



Scan time 02:42

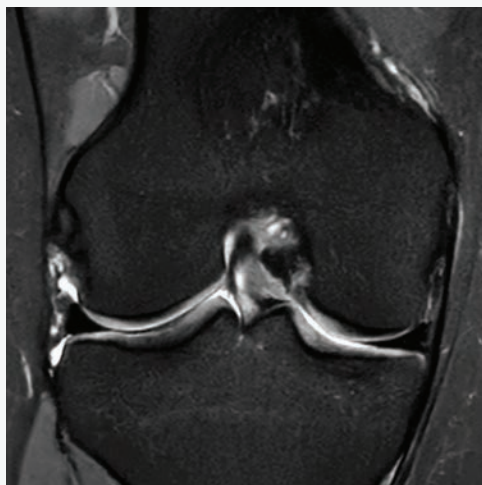

Scan time 01:36

### Knee PDWI FS

3.0T  
Philips  
Ingenia CX

2D TSE  
Ⓐ 0.4×0.5×3.0 mm  
Ⓑ 0.4×0.5×3.0 mm

\* For investigational purposes in countries outside of the United States, South Korea, Canada, Brazil, Japan, Taiwan, Malaysia, Saudi Arabia, UAE, Thailand, Vietnam, and Indonesia. FDA 510(k)-cleared to support images with scan time reduction by up to 50% in the United States.




---


**Breast  
T2WI FS**

**3.0T  
Philips  
Ingenua CX**

2D TSE  
Ⓛ 1.4×1.5×1.0 mm  
Ⓡ 1.2×1.3×1.0 mm

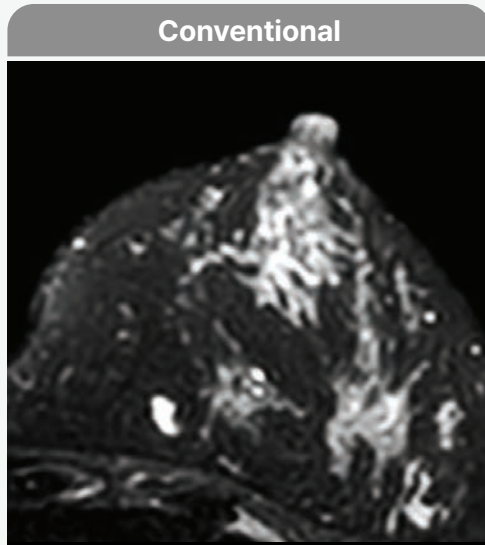

Scan time 05:14

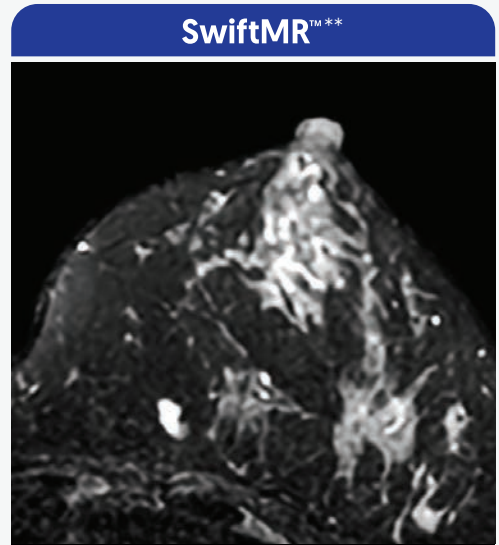


Scan time 03:17

---


**Breast  
DWI b800**

**3.0T  
Philips  
Ingenua CX**

2D EPI Diffusion  
Ⓛ 1.3×1.3×3.0 mm  
Ⓡ 1.3×1.3×3.0 mm

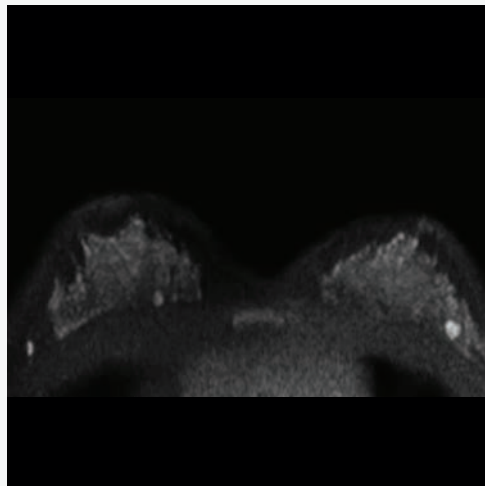

Scan time 06:31

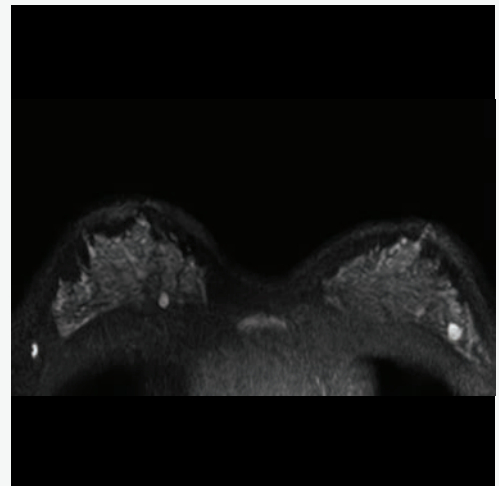


Scan time 04:43

---


**Heart  
CINE**

**3.0T  
Siemens  
MAGNETOM Skyra**

2D TRUFL  
Ⓛ 1.4×2.2×6.0 mm  
Ⓡ 1.4×1.8×6.0 mm

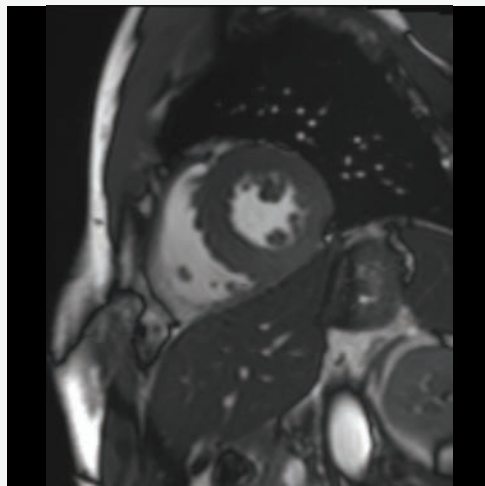

Scan time 01:29

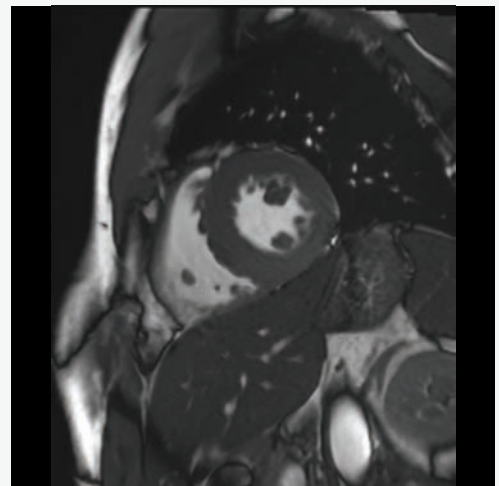

Scan time 00:55

---

\* FDA 510(k)-cleared for Standard of Care(SOC) and reduced scan time MR images for all body parts.


\*\* For investigational purposes in countries outside of the United States, South Korea, Canada, Brazil, Japan, Taiwan, Malaysia, Saudi Arabia, UAE, Thailand, Vietnam, and Indonesia. FDA 510(k)-cleared to support images with scan time reduction by up to 50% in the United States.



See more images




### Conventional

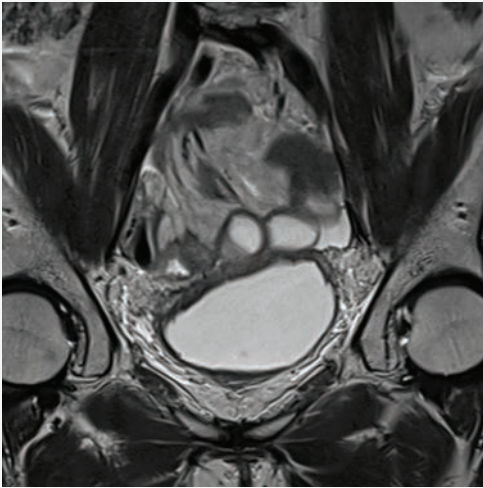

Scan time 03:51

### SwiftMR™\*

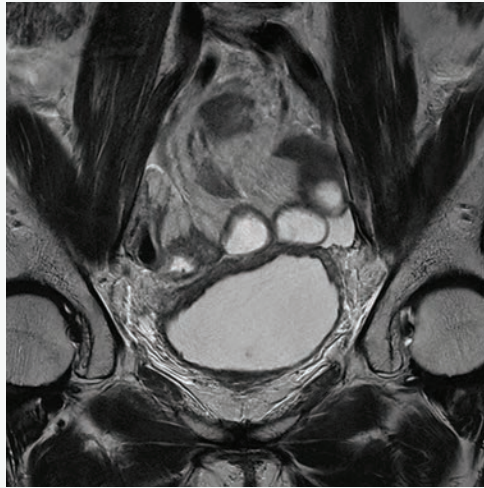


Scan time 02:41


## Bladder COR T2

3.0T  
Siemens  
MAGNETOM Skyra

2D TSE  
Ⓐ 0.6×0.9×3.0 mm<sup>3</sup>  
Ⓑ 0.5×0.7×3.0 mm<sup>3</sup>

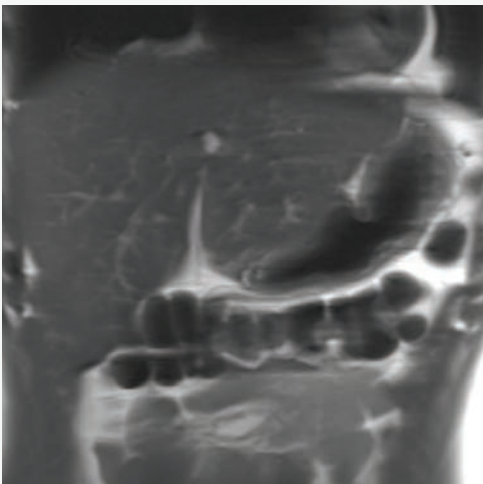

Scan time 00:33  
2 breath-hold

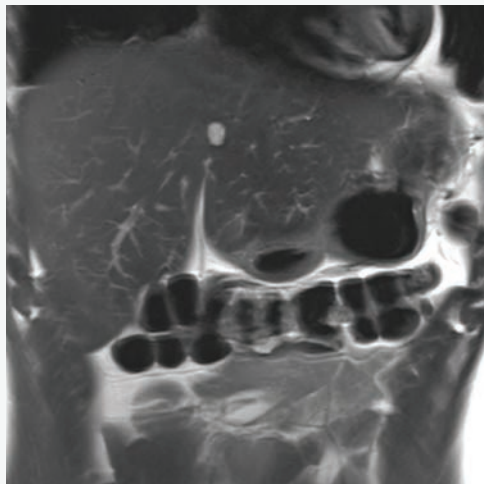


Scan time 00:17  
1 breath-hold


## Liver T2WI

3.0T  
Siemens  
MAGNETOM Skyra

2D HASTE  
Ⓐ 1.2×1.5×5.0 mm  
Ⓑ 1.0×1.2×5.0 mm

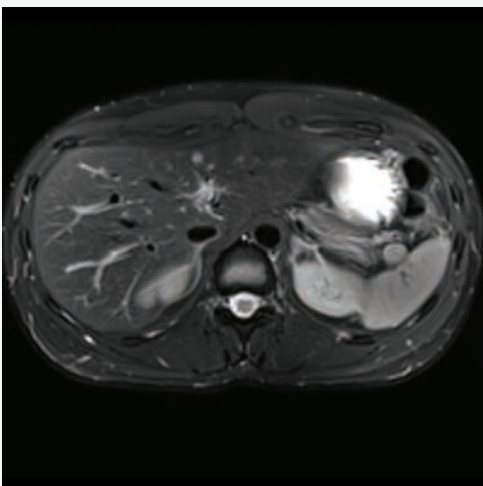

Scan time 02:20

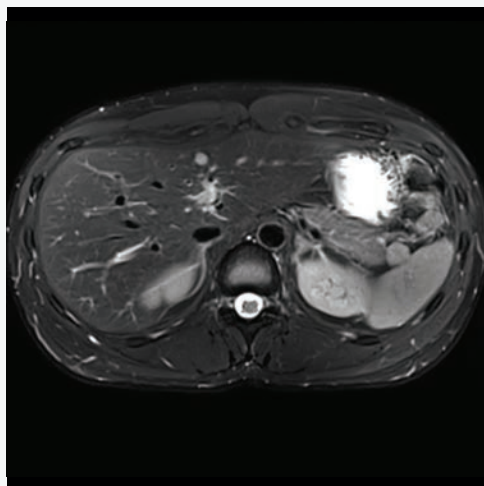

Scan time 01:45

## Liver T2WI FS

3.0T  
Siemens  
MAGNETOM Skyra

2D TSE-BLADE  
Ⓐ 1.5×1.5×4.0 mm  
Ⓑ 1.2×1.2×4.0 mm

# SwiftMR™ Improves Image Quality


SwiftMR™ enhances image quality, making scans even from legacy systems clearer and more detailed.

---


## Shoulder T2WI FS

1.5T  
Canon  
Vantage Elan

2D FSE  
0.5×0.8×3.0 mm  
Same scan

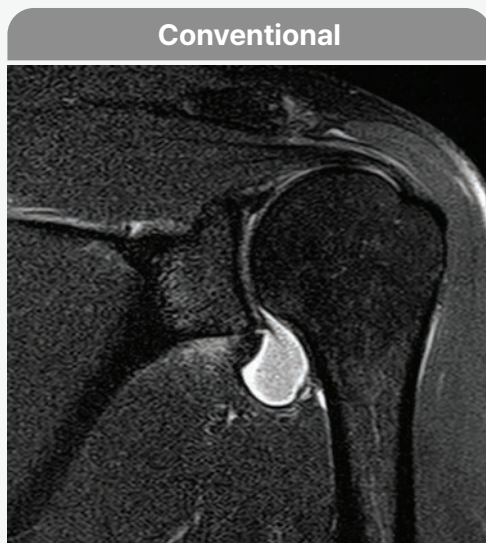

Scan time 02:12

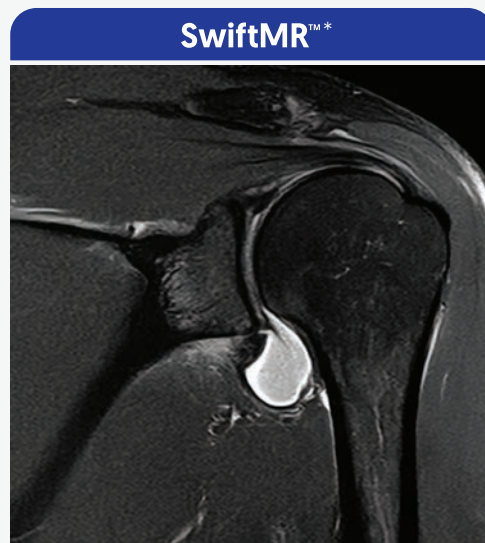

Scan time 02:12

---


## Knee STIR

0.6T  
FONAR  
UPRIGHT Multi-Position MRI

2D FSE  
0.8×0.8×4.0 mm  
Same scan



Scan time 05:26

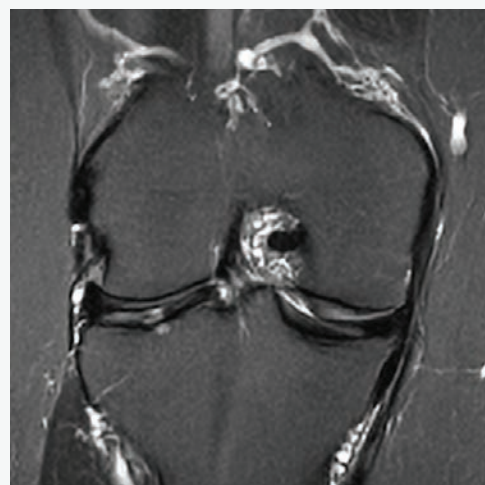


Scan time 05:26

---


## C-Spine T2WI

0.3T  
Hitachi  
AIRIS II

3D PBSG  
1.0×1.2×3.5 mm  
Same scan

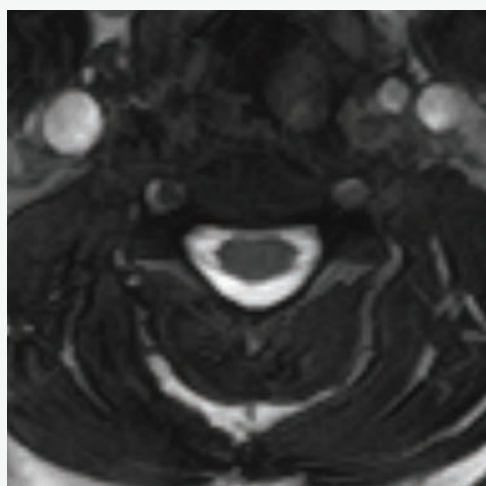

Scan time 03:24

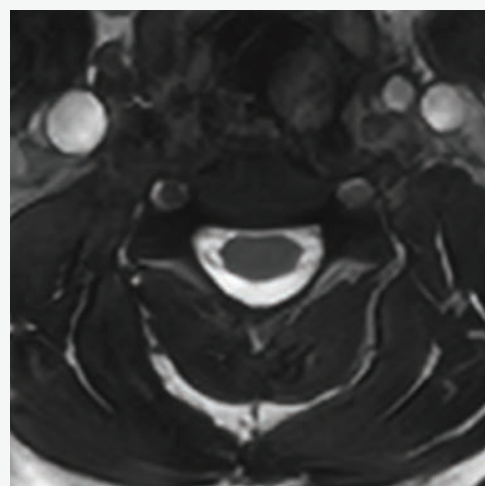


Scan time 03:24



# SwiftMR™ 's Seamless Integration

SwiftMR™ fits right into your existing system - no disruptions, no additional equipment required. We will provide a dedicated customer success team of MR experts to install our software and optimize your protocols.

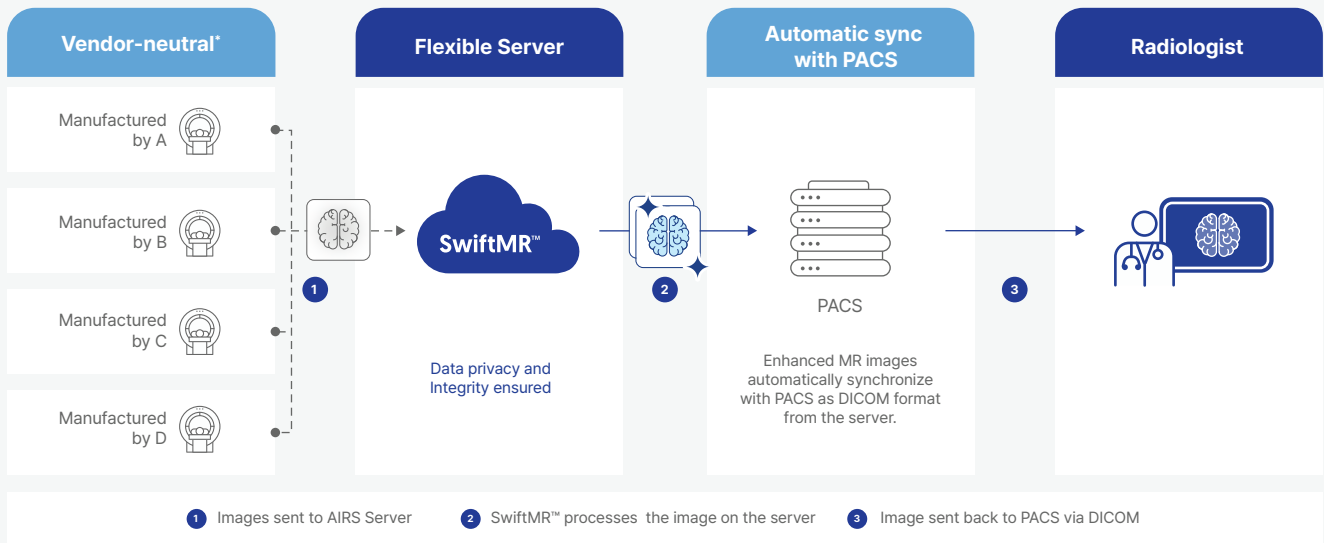

Supported body parts, pulse sequence, field strength, patient population and MRI manufacturers may vary by country

## Experience SwiftMR™ Firsthand

### Message from the CEO

In today's competitive healthcare landscape, choosing the right technology partner is crucial for success. As a growing AI company, we understand your concerns about trusting new solutions, especially in the sensitive domain of healthcare. Here at AIRS Medical, we prioritize building trust and ensuring the reliability of our AI-powered radiology solutions.

We are proud of SwiftMR™ positively impacting over 1 million patients globally, gaining accolades from radiologists, imaging specialists, and hospital administrators. The milestone underlines the efficacy and reliability of our technology.

We believe in putting our solutions to the test. **That's why we offer a 30-day limited trial of SwiftMR™.** This allows you to witness firsthand the improvements it can bring to your operations.



**Hye Seong Lee**  
AIRS Medical CEO

If you are interested in learning more about SwiftMR™, email us at [contact@airsmmed.com](mailto:contact@airsmmed.com) or visit our site via QR code at [airsmmed.com/en](https://airsmmed.com/en). We look forward to connecting with you.



Contact us

This document is for use by healthcare professionals only

DOC2382 (Rev.1)



MXR Corporate Headquarters:  
4909 Murphy Canyon Road  
Suite 120  
San Diego CA 92123

Call Us (888) 278-9933  
[customerservice@mxrimaging.com](mailto:customerservice@mxrimaging.com)



Visit our website